


# TCS-GSGSG-0225-0325 Calibration Substrate





The MPI TITAN™ TCS-GSGSG-0225-0325 Dual Calibration Substrate is designed to provide accurate probe tip calibration of MPI TITAN™ RF probes with ground-signal-ground-signal-ground (GSGSG) tips and the standard's layout is optimized implementing recommendations developed by the PlanarCal Consortium of twelve European organizations<sup>[1]</sup>. It supports the industry standard Short-Open-Load-Thru (SOLT/TOSM) calibration method, as well as advanced Thru-Match-Reflect (TMR/LRM), Thru-Match-Reflect-Reflect (TMRR) and the NIST multi-line Thru-Reflect-Line (mTRL) calibrations. The TCS-GSGSG-0225-0325 contains the full set of coplanar transmission lines for mTRL calibrations up to 110 GHz.

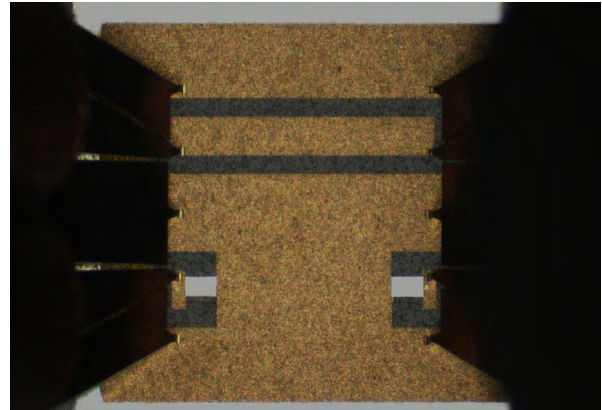

Two opposing GSGSG TITAN™ Dual Probes in separation after touching the Thru (Adj Load) Standard and using 10 μm vertical over-travel.

The unique approach of terminating idle RF probe ports by an Adjacent Load element implemented for MPI's TCS dual calibration substrates family drastically improves calibration accuracy at the mmW frequency range<sup>[2]</sup>.

## TYPICAL ELECTRICAL FIGURES

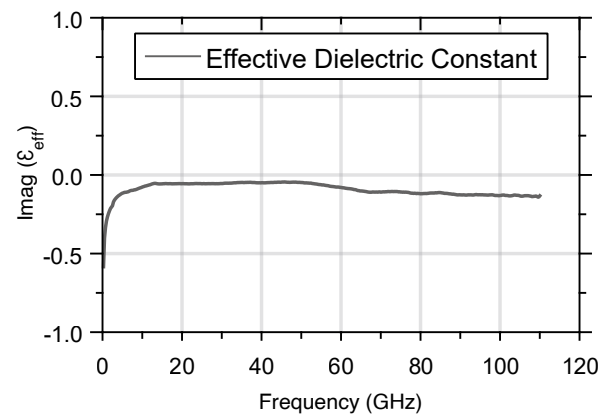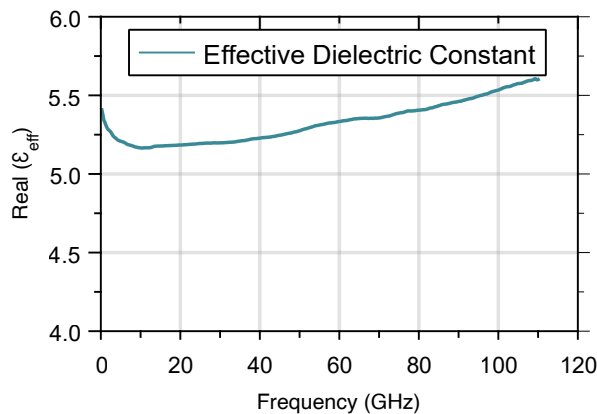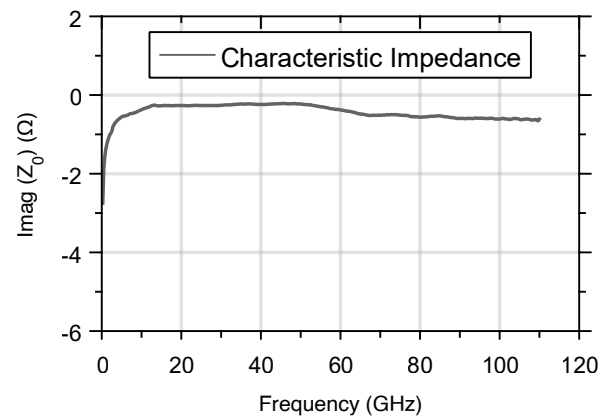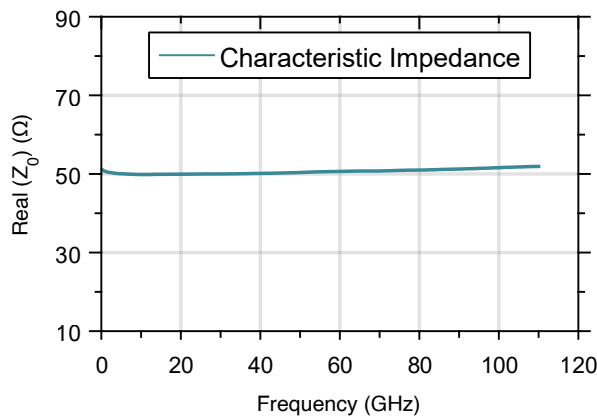

## SUBSTRATE CHARACTERISTICS

Material	Alumina
Size	16.7 mm x 12.7 mm
Thickness	254 $\mu$ m
Design or standards	Coplanar
Probe configuration	GSGSG
Supported probe pitch	225 to 325 $\mu$ m
Number of calibration and verification lines	3
Calibration verification elements	yes
Supported calibration methods	TOSM (SOLT), TMR, LRM, SOLR, TMRR, TRL and mTRL
Typical resistance of the load	50 $\Omega$
Typical load trimming accuracy error	$\pm$ 0.3 %
Open standard	Au pads on substrate
Recommended overtravel for TITAN™ probes	10 $\mu$ m


## ELECTRICAL CHARACTERISTICS OF CPW LINE STANDARDS

Nominal capacitance per unit length, pF/cm	1.52
Nominal characteristic impedance @20 GHz	50 $\Omega$
Effective dielectric constant @20 GHz, real part	5.31
Velocity factor @20 GHz	0.434
<b>Parameters of the simplified model of line losses</b>	
Reference loss, dB	0.26
Reference delay, ps	30
Reference frequency, GHz	30
<b>Electrical length of line, ps</b>	
Thru (Adj Load)	6.92
Thru (Adj Load) 1 (0201,0205)	10.14
Thru (Adj Load) 2 (0301,0305)	15.52
Thru (Adj Load) 3 (0401,0405)	29.81
Dual Thru (0103)	7.06
Vertical Thru (0402 - 0404)	4.73

**CALIBRATION ACCURACY USING NIST MULTILINE THRU-REFLECT-LINE (mTRL) PROCESS**

The mTRL calibration kit can be easily designed and fabricated using the same semiconductor process as the DUT. Customized "On-wafer" mTRL calibration kits eliminate the need for de-embedding the DUT measurement results from parasitic impedances of the device contact pads. The mTRL is the only method that delivers trustworthy calibration results at measurement frequencies above 220 GHz.

The mTRL algorithm requires multiple Line standards of different physical lengths and always treats the first Line (the "Thru") standard as a zero-length line. As a result, the length of each subsequent Line standard, Delta-l, is defined with respect to the length of the Thru (the first line).

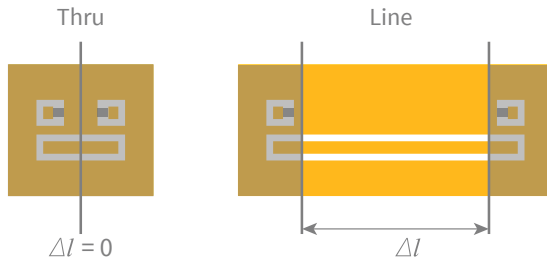

The TRL definition of the  $\Delta l$  for line standards



The MP80-DX MicroPositioner with the digital micrometer on the X axes.



Standard type, (Name)	Physical length, $\mu\text{m}$	Effective length l, $\mu\text{m}$	$\Delta l$ , $\mu\text{m}$
Thru (Adj Load)	950	900	0
Thru (Adj Load) Line 1 (0201,0205)	1370	1320	420
Thru (Adj Load) Line 2 (0301,0305)	2070	2020	1120
Thru (Adj Load) Line 3 (0401,0405)	3930	3880	2980

**PROBE TIP POSITIONING AND ALIGNMENT MARKS**

Consistent and accurate placement of the probe tips on calibration structures is critical for accurate and repeatable system calibration. The MPI TITAN™ TCS calibration substrate simplifies correct probe-tip-to-structure-alignment by providing special pre-alignment structures for the end user. The pre-alignment structures (Alignment Marks) enable the user to contact the Short, Open, Load and Thru structures in the correct location for consistent calibration results. For the Short, Open and Load, correct alignment is at the middle of each pad (Y-axis or relative to the direction of probe tip skate). For the Thru/Line elements, the correct alignment is 10-15  $\mu\text{m}$  inward from each end of line so the two opposing probes are apart by the specified distance that corresponds to the effective length of the element.

The unique saw-tooth like Alignment Marks (structures # 0602-0604) and cone-shaped Outer Marker found on the TCS calibration substrate are designed for proper probe-tip-to-calibration-structure edge adjustment. The edge of the Alignment Marks (as highlighted by the red dashed line in Figure below) corresponds to the endpoint on a Short, Open, Load or Thru/Line structure when the proper amount of probe overtravel and resulting 10-15  $\mu\text{m}$  of probe tip skate has been used. Skate begins from the moment the probe tips first make contact to the substrate (See the blue dashed line in Figure below) where initial tip contact should occur.

The operator should aim for and use the blue dashed line and cone of the Outer Marker as a visual reference/starting point for 10-15  $\mu\text{m}$  of probe tip skate. Minimal vertical overtravel (less than 20  $\mu\text{m}$  typically) is needed so the tips skate from the blue dashed line (outside saw tooth opening) to the red dashed line (at the edge, but not into the saw tooth opening) as the stopping point. When done properly, two opposing probes are at the correct physical distance and rotational alignment when both are resting at the red dashed line in the example (at the edge of, but not inside, the saw tooth openings on the Alignment Marks).

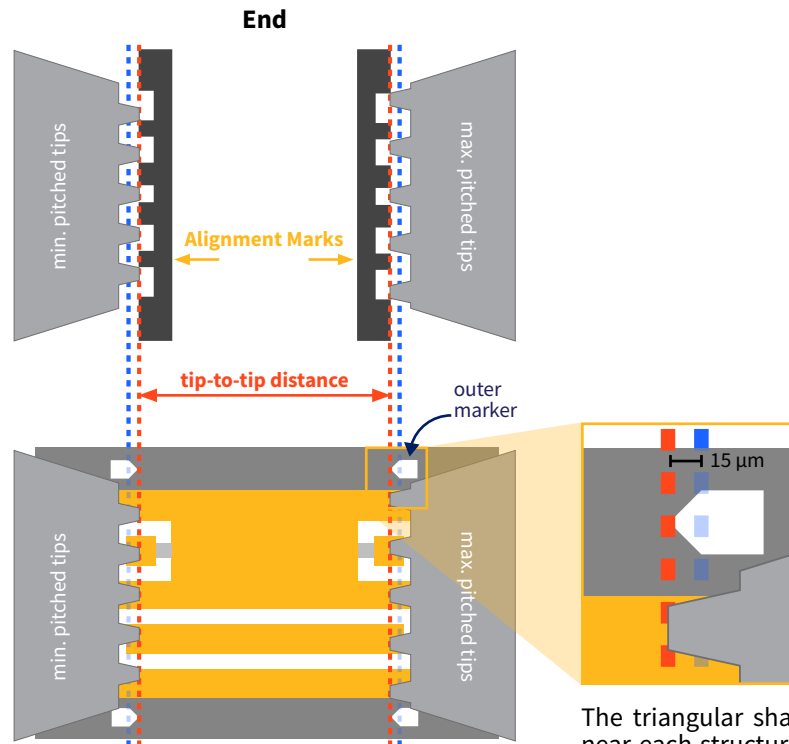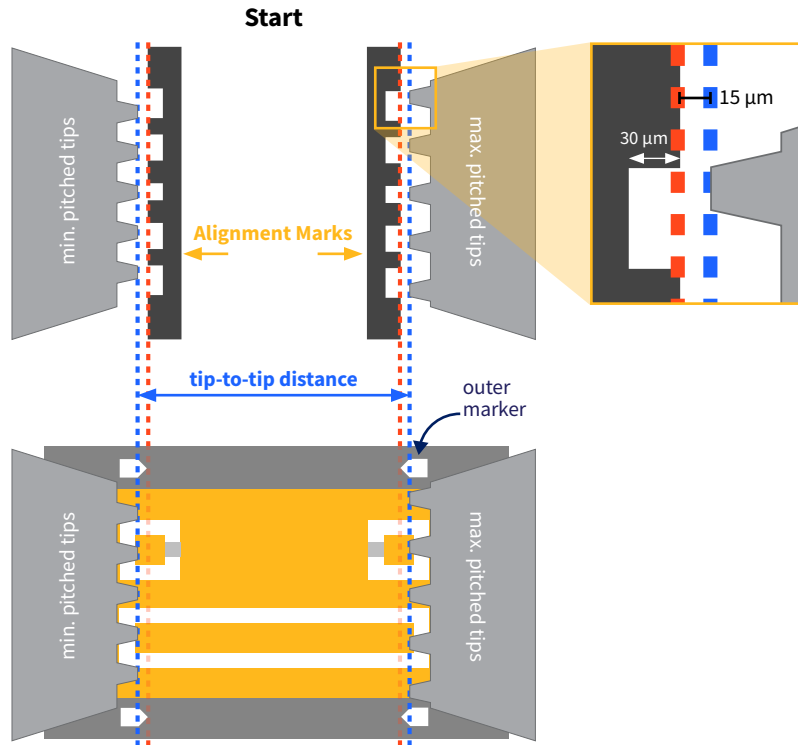

The triangular shaped marker located near each structure provides a measurable visual reference for the 15 µm of skate and proper tip placement.


**SUBSTRATE LAYOUT**



\*Location reference elements is 0102.


**STANDARD ELEMENTS**


**Standards with adjacent loads**

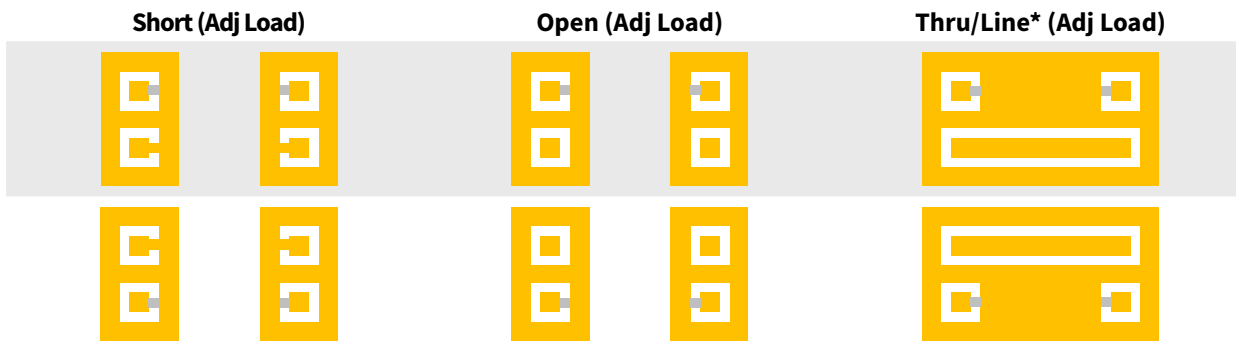

\*Lines: three choices of transmission lines provided, each with different physical and electrical lengths.

**Dual standards**

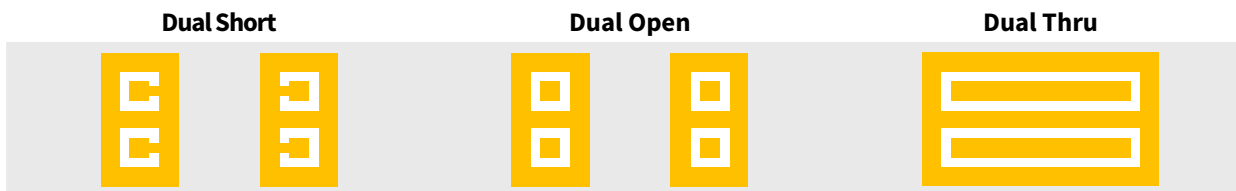

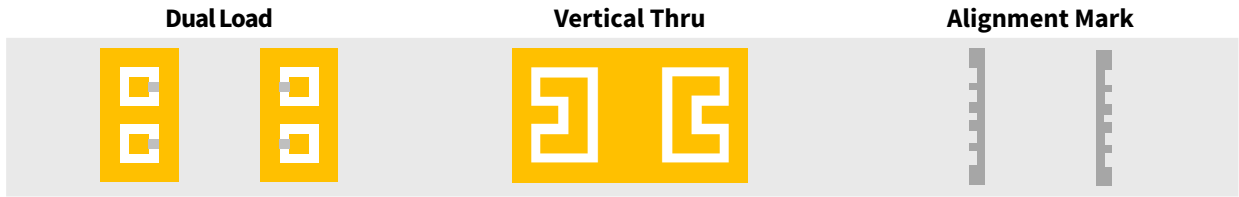


**AUTOMATED NAVIGATION IN SENTIO®**






SENTIO® probe station software from MPI Corporation is powerful Graphical User Interface (GUI) software to take your semiconductor testing to the next level. With unparalleled usability, multi-touch capabilities, and a customizable dashboard, SENTIO® software is designed to make your testing and microwave probe calibration processes more efficient and productive. Picture in Picture and QAlibria® inside provide advanced data analysis tools, while built-in intelligence streamlines your testing processes and keeps your probes and devices safe.

Connectivity and upgradability mean you're always connected and up to date with the latest features, while scalability ensures that SENTIO® software can grow with your business.

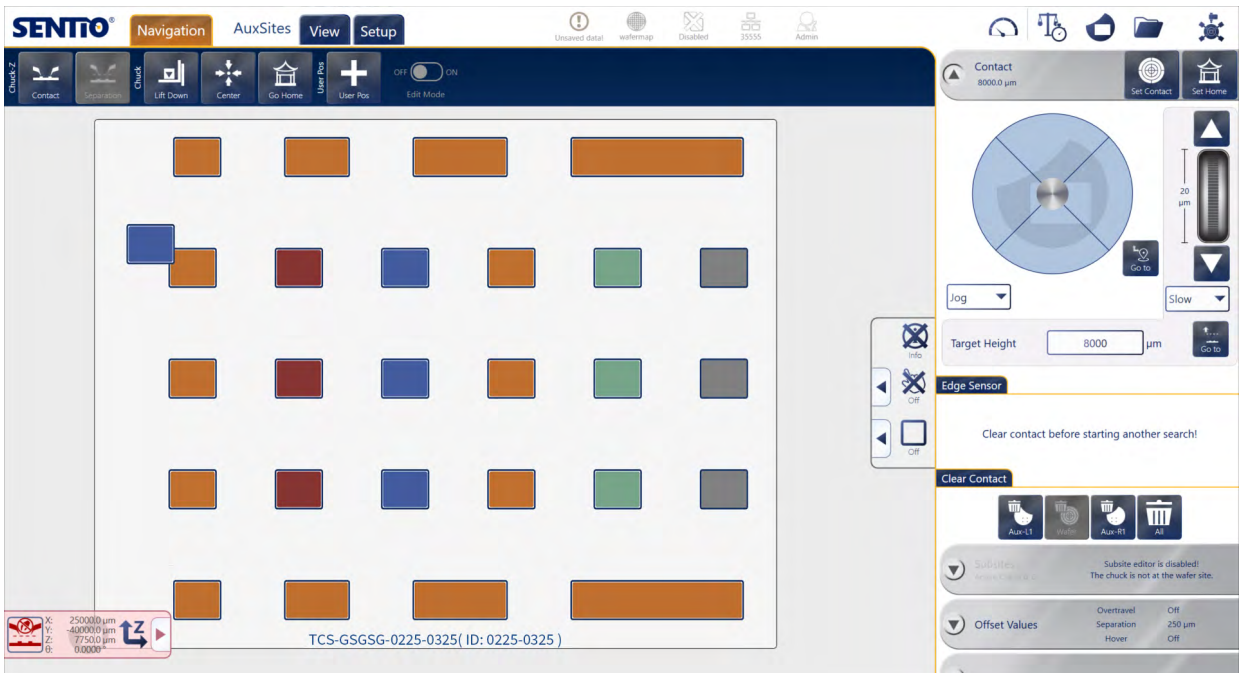SENTIO® and QAlibria® integrate seamlessly with the structure mapping of your TCS calibration substrate, making standards navigation the calibration process automated and easy even for inexperienced operators.

**The map of the TCS-GSGSG-0225-0325 substrate in SENTIO®**



-  Thru (Adj Load), Dual Thru, Vertical Thru, Line (Adj Load)
-  Short (Adj Load), Dual Short
-  Open (Adj Load), Dual Open, Open on bare ceramic or in Separation
-  Dual Load
-  Alignment Mark

## STANDARDS

### Thru Standards with Adjacent Load

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0102	Thru (Adj Load)	0	0	900
0104	Thru (Adj Load)	0	-4680	900
0101	Thru (Adj Load)	110	2340	900
0105	Thru (Adj Load)	110	-7020	900

### Line Standards with Adjacent Load

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0201	Line1 (Adj Load)	2750	2340	1320
0301	Line2 (Adj Load)	5810	2340	2020
0401	Line3 (Adj Load)	9570	2340	3880
0205	Line1 (Adj Load)	2750	-7020	1320
0305	Line2 (Adj Load)	5810	-7020	2020
0405	Line3 (Adj Load)	9570	-7020	3880

### Short Standards with Adjacent Load

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0202	Short (Adj Load)	2530	0	900
0204	Short (Adj Load)	2530	-4680	900

### Open with Adjacent Load

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0302	Open (Adj Load)	5060	0	900
0304	Open (Adj Load)	5060	-4680	900

### Dual Calibration Standards

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0103	Dual Thru	0	-2340	900
0203	Dual Short	2530	-2340	900
0303	Dual Open	5060	-2340	900
0502	Dual Load	10120	0	900
0503	Dual Load	10120	-2340	900
0504	Dual Load	10120	-4680	900

### Vertical (Loop-Back) Thru Standards

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0402	Vertical Thru	7590	0	900
0403	Vertical Thru	7590	-2340	900
0404	Vertical Thru	7590	-4680	900



**Probe Alignment Elements**

Name	Type	X $\mu\text{m}$	Y $\mu\text{m}$	Spacing $\mu\text{m}$
0602	Alignment Mark	12650	0	900
0603	Alignment Mark	12650	-2340	900
0604	Alignment Mark	12650	-4680	900

**CALIBRATION COEFFICIENTS FOR THE TITAN™ DUAL PROBES****GSGSG Configuration**

Pitch	Model	C-Open, fF	L-Short, pH	L-Term, pH
225 $\mu\text{m}$	26, 40, 50 GHz, Standard	9.0	81	66
250 $\mu\text{m}$	26, 40, 50 GHz, Standard	8.5	81	68
325 $\mu\text{m}$	26, 40, 50 GHz, Standard	9.2	87	73

**GSGSG Configuration, for the Keysight VNA**

Pitch	Model	C-Open, fF		L-Short, pH			Load*	
		C, fF	L, pH	R, Ohm	Offset $Z_0$ , Ohm	Offset delay, ps		
225 $\mu\text{m}$	26, 40, 50, 67 GHz, Standard	9.0	81	50	500	0.133		
250 $\mu\text{m}$	26, 40, 50, 67 GHz, Standard	8.5	81	50	500	0.137		
325 $\mu\text{m}$	26, 40, 50, 67 GHz, Standard	9.2	87	50	500	0.147		

\*Use both offset impedance and offset delay parameters.

**REFERENCES**

- [1] M. Spirito, U. Arz, G. N. Phung, F. J. Schmückle, W. Heinrich, and R. Lozar, "Guidelines for the design of calibration substrates, including the suppression of parasitic modes for frequencies up to and including 325 GHz," in "EMPIR 14IND02 – PlanarCal," Physikalisch-Technische Bundesanstalt (PTB), 2018.
- [2] H.-C. Fu, K. Jung. "Improve RF Dual Probe Calibration Accuracy with Peer-Terminated Standard", in 2024 IEEE / MTT-S International Microwave Symposium - IMS 2024, Washington, DC, USA, 16-24 June, 2024.

See MPI Corporation's Terms and Conditions of Sale for more details.

Direct contact:  
 Asia region: ast-asia@mpi-corporation.com  
 EMEA region: ast-europe@mpi-corporation.com  
 America region: ast-americas@mpi-corporation.com

MPI global presence: for your local support, please find the right contact here:  
[www.mpi-corporation.com/ast/support/local-support-worldwide](http://www.mpi-corporation.com/ast/support/local-support-worldwide)

**MPI Global Presence**